



Publication number : **0 542 422 A1**

EUROPEAN PATENT APPLICATION

Application number : **92309172.2**

Int. Cl.⁵ : **B01L 3/00, B01L 7/00**

Date of filing : **08.10.92**

Priority : **12.11.91 US 790365**

Date of publication of application :
19.05.93 Bulletin 93/20

Designated Contracting States :
CH DE FR GB LI

Applicant : **GENERAL ATOMICS**
3550 General Atomics Court
San Diego, California 92121 (US)

Inventor : **Garner, Harold R.**
1626 Gitano Street
Encinitas, California 92024 (US)
Inventor : **Shepherd, Glen**
7408 Carlina Street
Carlsbad, California 92008 (US)

Representative : **Coxon, Philip et al**
Eric Potter & Clarkson St. Mary's Court St.
Mary's Gate
Nottingham NG1 1LE (GB)

Multi-well microtiter plate.

(57) A system and method for the high volume processing of a plurality of minute liquid specimens uses a multi-well microtiter tray (12) which has a base (14) with a flat underside and a plurality of wells (18) that are formed on the base. As intended for the present invention there are eight hundred and sixty four wells formed on the base (14). Also, included in the system is a structure which has a heat transfer plate (34) for supporting the microtiter tray (12), and for effecting heat transfer with the liquid specimens in the wells (18) of the tray (12). In one embodiment, the plate itself functions as a heat source. Alternatively, the plate functions as a heat sink and a heating element mounted on the structure is employed to heat the liquid specimens which are held in the wells of the tray. For this alternative embodiment, operation of the plate can be controlled in concert with the operation of the heating element. By controlling the operations of the plate and the heating element, the system of the present invention can cyclically vary the heating of the liquid specimens for procedures such as DNA amplification. The base of the tray, and the bottoms of the wells in the base of the tray, are light transparent to selectively allow simultaneous photometric or fluorometric measurements of all liquid specimens being held on the microtiter tray.

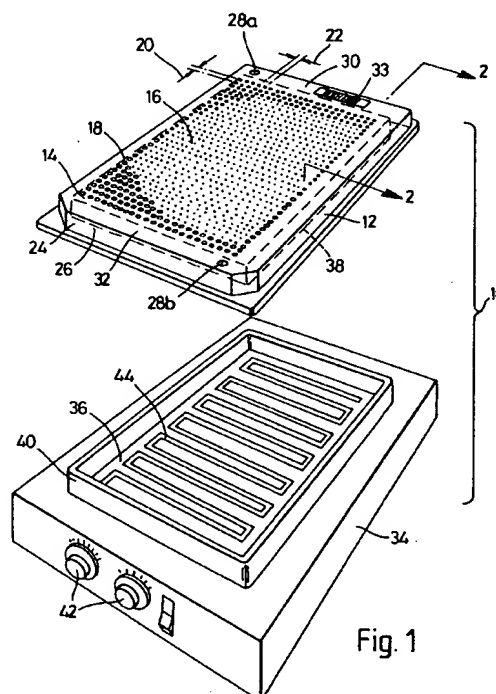


Fig. 1

FIELD OF THE INVENTION

The present invention generally pertains to multi-well microtiter trays which are useful for holding a plurality of minute liquid samples. More particularly, the present invention pertains to microtiter trays which can hold a plurality of liquid specimens while they are being cultivated by a temperature varying regimen and during periodic photometric or fluorometric measurements of the specimens. The present invention is particularly, but not exclusively, useful for DNA amplification and sequencing.

BACKGROUND OF THE INVENTION

The laboratory processing of liquid samples has been accomplished in the past for many varied purposes. Examples of these purposes include cultivating cells in the specimens, transferring and storing the specimens, and using the liquid specimens for forensic purposes or to diagnose a diseased condition. Not unexpectedly, with advances in science the number and variety of such procedures is increasing and, in many instances, the procedures themselves are more complex and require increased precision. For one thing, this means that proper equipment must be used which is capable of performing the particular procedure with the required precision. Further, it means that the equipment must also be capable of efficaciously handling the liquid sample. And, in some cases, the ability of the equipment to handle the liquid sample may be no small matter. As is well known, many procedures require individual processing of a very large number of discrete liquid samples under the same or very similar conditions. Moreover, where expense is an overriding concern, additional factors need to be considered.

In instances where the cost of the sample material is significant, such as would clearly be the case for the processing of DNA specimens, there is a compelling interest to use as little of the material as is possible. For expensive sample material this interest is even more acute in instances where it is necessary to process a very large number of discrete specimens of the sample material. Accordingly, there is a need for laboratory equipment which can efficaciously handle a relatively large volume of sample material as a large number of discrete and relatively minute specimens.

Microtiter trays with many wells for separately receiving liquid specimens have been used in the past to hold and store small specimens of sample material. Typically, these earlier trays have been designed for use with robotics which are capable of engaging the microtiter tray to deposit the specimens in the wells of the tray. In practice, the industry standard has been to provide microtiter trays which are separated by a center-to-center distance of nine millimeters. Accordingly, the robotics which are used with currently

available microtiter trays have been designed to comply with this standard. This restriction on spacing between the wells of the tray can be perceived as a disadvantage if the desire is to process as many discrete samples as possible. There are, however, other potential disadvantages in presently available microtiter trays.

In light of relatively recent advancements in specific areas of science, such as the processing of DNA samples, it is often desirable to have several functions accomplished while the liquid specimen remains in the well of the microtiter tray. For example, in the process of DNA amplification or sequencing, it is necessary for the liquid specimen to be subjected to a cyclical temperature regimen. Further, again for DNA amplification, it is desirable to periodically evaluate the specimen and determine whether the process is being accomplished successfully. It happens that this evaluation can be effectively done by taking photometric or fluorometric measurements of the liquid specimens. Thus, there is a need for a multifunctional microtiter tray. Specifically, in addition to providing increased storage capacity and enhanced ease in handling minute liquid specimens, it is desirable to have a microtiter tray which can be used in processes which vary and maintain the temperature of the specimens according to predetermined temperature regimens, and which can be used during photometric or fluorometric analysis of the specimens.

In light of the above it is an object of the present invention to provide a multi-well microtiter tray which is useful for simultaneously processing a high volume of minute liquid samples. Another object of the present invention is to provide a multi-well microtiter tray which is efficient in handling a very large number of individual minute liquid specimens. Yet another object of the present invention is to provide a multi-well microtiter tray which is useful with robotics which function in accordance with existing standards of the industry. Still another object of the present invention is to provide a multi-well microtiter tray which minimizes the storage space which is required for a very large number of minute liquid specimens. Another object of the present invention is to provide a multi-well microtiter tray which allows for substantially even heating of all liquid specimens being held in the tray. Yet another object of the present invention is to provide a multi-well microtiter tray which has sufficiently good optical qualities to allow for simultaneous photometric or fluorometric measurements of the liquid specimens in the tray. Yet another object of the present invention is to provide a multi-well microtiter tray which is simple to use, relatively easy to manufacture and comparatively cost effective.

SUMMARY OF THE INVENTION

A multi-well microtiter tray for use in a system, or

in a method, for high volume processing of a plurality of minute liquid specimens includes a generally rectangular base having a substantially flat underside. The top of the base is formed with a very large number of wells for holding a very large number of individual liquid specimens. As specifically intended for the present invention, the top of the microtiter tray is formed with eight hundred and sixty four wells which are arranged in a rectangular array that is thirty-six by twenty-four. Each well in the array has an opening and a bottom and is substantially cylindrical shaped to define a curved wall which tapers inwardly from the opening of the well to the bottom of the well. The bottom of each well is distanced from the underside of the base and has an optical quality surface for transmitting light through the underside and through the liquid specimens held in the well. The bottom of each well may be either flat, or rounded, or cone-shaped.

The system for using the multi-well microtiter tray includes a support structure which has a heat exchanger that is engageable with the microtiter tray. In one embodiment of the present invention, the heat exchanger is a heat source which conductively transfers heat to the liquid specimens in the well through the base of the microtiter tray. In another embodiment of the present invention, the heat exchanger acts as a heat sink and the support structure further includes a heating element. As one example, this heating element may be a heat radiator such as would be the case for a microwave oven. Preferably, however, the heating element comprises a plurality of heating probes which can be inserted into selected wells of the microtiter tray to conduct heat through the tray to the other wells in the microtiter tray. For the embodiments where the heat exchanger is to be used as a heat sink, the system can also include a controller to coordinate the operation of the heating element with the operation of the heat exchanger to cycle the liquid specimens through predetermined temperature regimens.

Due to the construction of the base of the microtiter tray, light can be transmitted through the liquid specimens for photometrically or fluorometrically measuring the characteristics of the liquid specimens. This can be simultaneously done for all of liquid specimens held by the microtiter tray as they are being processed. Processes which can be accomplished using the system and methods for using a microtiter tray as intended for the present invention include DNA amplification sequencing and library construction.

The novel features of this invention, as well as the invention itself, both as to its structure and its operation will be best understood from the accompanying drawings, taken in conjunction with the accompanying description, in which similar reference characters refer to similar parts, and in which:

BRIEF DESCRIPTION OF THE DRAWINGS

Figure 1 is an exploded perspective view of the system of the present invention;

Figure 2A is a cross-sectional view of the preferred embodiment of the wells in the microtiter tray of the present invention as seen along the line 2-2 in Figure 1 shown schematically with a device for photometrically or fluorometrically measuring liquid specimens in the wells;

Figure 2B is a cross-sectional view of another embodiment of the wells in the microtiter tray of the present invention as would be seen along the line 2-2 in Figure 1;

Figure 2C is a cross-sectional view of yet another embodiment of the wells in the microtiter tray of the present invention as would be seen along the line 2-2 in Figure 1;

Figure 2D is an enlarged cross-sectional view of the preferred embodiment of the wells in the microtiter tray of the present invention as seen along the line 2-2 in Figure 1 showing dimensions for the wells and the engagement of a well in the microtiter tray with a probe;

Figure 3 is a perspective view of the system of the present invention in an operational environment with a robot;

Figure 4 is a perspective view of the system of the present invention operatively positioned for use with a microwave oven;

Figure 5 is a perspective view of the microtiter tray of the present invention engaged with a heat transfer tool;

Figure 6 is a cross-sectional view of the microtiter tray as seen along the line 6-6 in Figure 5;

Figure 7 is a perspective view of the system of the present invention in use with a probe heater; and Figure 8 is a cross-sectional view of the microtiter tray engaged with a probe heater as seen along the line 8-8 in Figure 7.

DESCRIPTION OF THE PREFERRED EMBODIMENTS

Referring initially to Figure 1, the system for high volume processing a plurality of minute liquid specimens, is shown and generally designated 10. As shown, the system 10 includes a microtiter tray 12 which has a base 14. Formed into the top surface 16 of the base 14 are a plurality of wells 18. Specifically, as intended for the present invention, base 14 of microtiter tray 12 is formed with eight hundred and sixty four (864) wells 18 which are arranged in a rectangular array that is thirty-six by twenty-four (36X24). The center-to-center distances 20 and 22 between the rows and lines of the wells 18 are set at three millimeters (3mm). Additionally, it will be appreciated by reference to Figures 2A, 2B, 2C and 2D, in addition

to Figure 1, that base 14 is of a solid construction. Stated differently, there is no space between the wells 18. Instead, the material of base 14 fills what could otherwise be empty space between the wells 18. This construction helps provide temperature uniformity for all of the liquid specimens held in the wells 18 because base 14 establishes a shorter thermal path from a well 18 to another well 18 to facilitate heat transfer therebetween.

Preferably, microtiter tray 12 is made of an optically clear rigid plastic such as polystyrene, polypropylene, or polycarbonate. Additionally, the plastic of tray 12 can include carbon fibers, alumina, aluminum oxide, or other metals which will enhance the thermal conductivity of the tray 12 but which will not interfere with its biological performance. As intended for the present invention, the tray 12 can be manufactured by any process well known in the pertinent art, such as by injection molding.

Figure 1 also shows that microtiter tray 12 has an overhang 24 which forms a detent 26 between the overhang 24 and the base 14 of tray 12. Additionally, a pair of registration points 28a and 28b can be formed into top surface 16 of tray 12 in order to align the tray 12 with a robot (not shown in Figure 1) for purposes to be discussed below. Also, the top surface 16 of microtiter tray 12 has a flat area 30 and a flat area 32 on which an identification strip, such as bar code 33, can be placed. As will be appreciated by the skilled artisan, some ability to identify the microtiter tray 12 and the liquid specimens held in the wells 18 of the tray 12 can be essential.

As shown in Figure 1, the system 10 of the present invention includes a support structure on which microtiter tray 12 can be placed. At this point it is to be noted that, within the contemplation of the present invention, the support structure may be merely a storage shelf. For example the support structure may be part of a library for biological specimens, such as a shelf in a standard refrigerator (not shown) or an incubator (not shown). Regardless, in addition to the specific support structures disclosed below, it is intended that the support structure may encompass any platform where the microtiter tray 12, and the liquid specimens in the wells 18 of tray 12, can be stored for prolonged periods of time. In addition to the storage function of any particular support structure, a more operational function is for heat transfer with the liquid specimens. Specifically, when processing liquid specimens in the wells 18 of microtiter tray 12, the support structure is as a heat exchanger 34.

For the purposes of the present invention, heat exchanger 34 can be either a heat source or a heat sink. In either case, it must be operatively engageable with the microtiter tray 12. For the embodiment of heat exchanger 34 shown in Figure 1, heat exchanger 34 can have a surface 36 which will directly abut against the flat underside 38 of base 14 of the micro-

titer tray 12. Though not shown, it will be appreciated by the skilled artisan that a thermal grease, or some other such substance well known in the pertinent art can be placed on the surface 36 to facilitate heat transfer between the heat exchanger 34 and the microtiter tray 12. An additional feature of the system 10 of the present invention which promotes good heat transfer characteristics for the microtiter tray 12 is that both the top surface 16 and underside 38 of the tray 12 are flat and each have a relatively large area. Additionally, heat exchanger 34 can be formed with a ridge 40 which is matingly received into the detent 26 of microtiter tray 12 to help hold the tray 12 in position on heat exchanger 34. For the embodiment of the system 10 wherein the heat exchanger 34 acts as a heat source, the exchanger 34 can include controls 42a,b for the purpose of precisely controlling the amount of heat which is to be applied from the heating coils 44 of heat exchanger 34 to the tray 12 during the processing of the liquid specimens in the wells 18.

Actual configurations for the wells 18 will be best appreciated with reference to the Figures 2A, 2B, 2C and 2D. There, and with cross reference to Figure 1, it will be appreciated that each of the wells 18 in microtiter tray 12 is essentially a hollow cylindrical recess which is formed into the top surface 16 of the tray 12. Specifically, each well 18 has an opening 46 and is defined by a cylindrical sidewall 48 which extends from the opening 46 to the bottom of the well. In Figure 2A, a well 18 is shown to have a substantially flat bottom 50, whereas in Figure 2B the well 18 has a rounded bottom 52, and in Figure 2C the well 18 is shown with a cone shaped bottom 54. According to the particular needs of the user, a particular shape for the bottom of well 18 may be preferable. For instance, the rounded bottom 52 of well 18 is better suited for use with liquid specimens which include cells which might tend to cling to the angled surfaces presented by a flat surface 50. Further, the cone-shaped surface 54 might be preferable for use with automatic pipetting.

Regardless of their particular configuration, the bottoms 50, 52, and 54 of wells 18, as well as underside 38 of base 14, must be optically clear. Stated differently, sufficient light with which to make photometric or fluorometric measurements of the liquid specimens 56 being held in the well 18 must be able to pass through underside 38, through the bottom 50, 52, 54 of well 18 and through the liquid specimen held in well 18. For the purposes of the present invention, optically clear means that the bottom 50, 52, or 54 has a smoothness such that deviations in their surface do not exceed more than one quarter wavelength of the light which is passed through tray 12 and the liquid specimen 56 to make photometric or fluorometric measurements of the liquid specimen 56. As intended for the present invention, and due in part to the plastic materials used for the manufacturing of tray 12, the

light used for photometric or fluorometric measurements of the liquid specimen 56 will be primarily in the visual range. The preferred dimensions for a typical well 18 will be best appreciated with specific reference to Figure 2D.

As indicated above, center-to-center distance 20 between adjacent wells 18 along either a line or a row of wells 18 is approximately three millimeters (3mm). Thus, a standard tool having a nine millimeter (9mm) spacing between probes can be used with the 3mm spacing of tray 12 if it is repeatedly used three times. This can be carried further. For example, in one embodiment for tray 12 the center-to-center distance can be four and a half millimeters (4.5mm). The standard robot would then need to be used twice. It happens that several configurations of the tray 12 can be used with standard robotics just so long as the center-to-center spacing is equal to nine divided by n, where n is an integer. Obviously, the volume capacity of the wells 18 will be sacrificed as more wells 18 and incorporated into the tray 12.

For a typical well 18 shown in Figure 2D, the diameter 58 of the opening 46 is approximately two millimeters (2mm). Though depicted with some exaggeration, Figure 2D shows that the sidewalls 48 of well 18 are tapered inwardly from the opening 46 of well 18 to its bottom 50. Specifically, the angle of taper 60 is approximately one degree (1°). The depth 62 of well 18 is approximately seven millimeters (7mm) with the result that well 18 is dimensioned to hold a liquid specimen 56 having a volume of approximately twenty microliters (20 ul). In many instances, however, the actual volume of the liquid specimen 56 which is to be deposited into a well 18 may have a liquid volume that is more on the order of one or two microliters (1-2 ul).

As is well known, liquid specimens which have total volumes on the order of one or two microliters can be hard to handle. A specific problem confronted by the present invention involves the transfer of such a small liquid specimen 56 into a well 18 of the microtiter tray 12. This problem stems from the fact that surface tension of the liquid specimen 56 will, at this level, be sufficient to prevent the specimen from forming into a drop which will fall into the well 18. Consequently, to assist the transfer of the liquid specimen 56 into the well 18, the sidewalls 46 of the well 18 are tapered.

Referring specifically to the well 18' shown in Figure 2D, it is contemplated by the present invention that a liquid specimen 56 will be transferred from a source of the liquid (not shown) to the well 18' of microtiter tray 12 by a device such as the probe 66. As stated above, the size of the liquid specimen 56 may be so small that it cannot form into a drop which will fall into the well 18'. However, since the sidewalls 48' of well 18' are tapered, probe 66 can be made to contact the sidewall 48' when it is inserted into the well 18'. This contact, a mere kiss if you will, is sufficient

to wet the sidewall 48' with the liquid specimen 56 and cause the liquid specimen 56 to flow into the bottom 50' of the well 18'.

Referring now to Figure 3, it will be seen that a robot 68 may be used to transfer liquid specimens 56 from a source of the specimens (not shown) to the microtiter tray 12. Specifically, the robot 68 is outfitted with an end effector 70 which has a plurality of probes 66 (e.g. eight hundred and sixty four) for this purpose. Each of the probes 66 is designed, in a manner well known in the pertinent art, to carry a minute quantity of a liquid specimen 56 for deposit on the tray 12. Further, the robot 68 can include well known means (not shown) on end effector 70 which will register with the registration points 28a,b on microtiter tray to properly align the probes 66 on end effector 70 with the wells 18 on microtiter tray 12. Though not shown, it will be appreciated that robot 68 is operable to engage end effector 70 with the microtiter tray 12 to deposit liquid specimens 18 in the wells 18 of tray 12.

Once the liquid specimens 56 have been deposited into the wells 18 of microtiter tray 12, heat exchanger 34 can be operated to heat the specimens 56 as desired by the user. This, of course, is for the embodiment of the system 10 wherein the heat exchanger 34 acts as a heat source. According to the present invention, various temperature regimens may be followed by the heat exchanger 34 when heating the specimens 56. DNA amplification is but one example of such a regimen.

Returning for the moment to Figure 2A, it will be seen that microtiter tray 12 is intended to be used during photometric or fluorometric measurements of the liquid specimens 56 which are deposited into the wells 18 of the tray 12. In Figure 2A a light source 72 is schematically shown in a relationship with the tray 12 for making such photometric or fluorometric measurements. The light source 72 may be of any type well known in the pertinent art, but it is preferably of a type which will emit a light 74 in the visual range having identifiable wavelengths, for example λ_1 . According to standard photometric or fluorometric analysis a resultant light 76 having a different wavelength, for example λ_2 , will result due to the particular characteristics of the liquid specimen 56. This resultant light 76 will then be received at a light detector 78 and the wavelength difference between light 74 and resultant light 76 can be used to measure the characteristics of the liquid specimen 56. As contemplated for the present invention, a photometric or fluorometric analysis of the liquid specimens 56 in microtiter tray 12 can be made at any time.

As indicated above, the heat exchanger 34 can be used as a heat sink as well as a heat source. Accordingly, when heat exchanger 34 is to a heat sink, another source of heat is needed for procedures wherein the liquid specimens 56 are to be cycled through a temperature regimen. Figure 4 indicates

that heat exchanger 34 can be incorporated as part of an oven 80 and that the microtiter tray 12 can be positioned on the exchanger 34 in oven 80. The door 82 of oven 80 can then be shut (not shown) to enclose microtiter tray 12 with its liquid specimens 56 inside the oven 80. Both the heating function of the oven 80, and the cooling function of the heat sink exchanger 34, can then be controlled from the control panel 84 to cycle the liquid specimens 56 in tray 12 through any temperature regimen desired by the user. As intended for the present invention, oven 80 may be of any type well known in the pertinent art. For example, oven 80 may be a microwave oven or it may be an air thermal cy-
 5

For those cases in which the oven 80 is an air thermal cy-
 10
 15
 20
 25
 30
 35
 40
 45
 50
 55
 60
 65
 70
 75
 80
 85
 90
 95
 100
 105
 110
 115
 120
 125
 130
 135
 140
 145
 150
 155
 160
 165
 170
 175
 180
 185
 190
 195
 200
 205
 210
 215
 220
 225
 230
 235
 240
 245
 250
 255
 260
 265
 270
 275
 280
 285
 290
 295
 300
 305
 310
 315
 320
 325
 330
 335
 340
 345
 350
 355
 360
 365
 370
 375
 380
 385
 390
 395
 400
 405
 410
 415
 420
 425
 430
 435
 440
 445
 450
 455
 460
 465
 470
 475
 480
 485
 490
 495
 500
 505
 510
 515
 520
 525
 530
 535
 540
 545
 550
 555
 560
 565
 570
 575
 580
 585
 590
 595
 600
 605
 610
 615
 620
 625
 630
 635
 640
 645
 650
 655
 660
 665
 670
 675
 680
 685
 690
 695
 700
 705
 710
 715
 720
 725
 730
 735
 740
 745
 750
 755
 760
 765
 770
 775
 780
 785
 790
 795
 800
 805
 810
 815
 820
 825
 830
 835
 840
 845
 850
 855
 860
 865
 870
 875
 880
 885
 890
 895
 900
 905
 910
 915
 920
 925
 930
 935
 940
 945
 950
 955
 960
 965
 970
 975
 980
 985
 990
 995
 1000
 1005
 1010
 1015
 1020
 1025
 1030
 1035
 1040
 1045
 1050
 1055
 1060
 1065
 1070
 1075
 1080
 1085
 1090
 1095
 1100
 1105
 1110
 1115
 1120
 1125
 1130
 1135
 1140
 1145
 1150
 1155
 1160
 1165
 1170
 1175
 1180
 1185
 1190
 1195
 1200
 1205
 1210
 1215
 1220
 1225
 1230
 1235
 1240
 1245
 1250
 1255
 1260
 1265
 1270
 1275
 1280
 1285
 1290
 1295
 1300
 1305
 1310
 1315
 1320
 1325
 1330
 1335
 1340
 1345
 1350
 1355
 1360
 1365
 1370
 1375
 1380
 1385
 1390
 1395
 1400
 1405
 1410
 1415
 1420
 1425
 1430
 1435
 1440
 1445
 1450
 1455
 1460
 1465
 1470
 1475
 1480
 1485
 1490
 1495
 1500
 1505
 1510
 1515
 1520
 1525
 1530
 1535
 1540
 1545
 1550
 1555
 1560
 1565
 1570
 1575
 1580
 1585
 1590
 1595
 1600
 1605
 1610
 1615
 1620
 1625
 1630
 1635
 1640
 1645
 1650
 1655
 1660
 1665
 1670
 1675
 1680
 1685
 1690
 1695
 1700
 1705
 1710
 1715
 1720
 1725
 1730
 1735
 1740
 1745
 1750
 1755
 1760
 1765
 1770
 1775
 1780
 1785
 1790
 1795
 1800
 1805
 1810
 1815
 1820
 1825
 1830
 1835
 1840
 1845
 1850
 1855
 1860
 1865
 1870
 1875
 1880
 1885
 1890
 1895
 1900
 1905
 1910
 1915
 1920
 1925
 1930
 1935
 1940
 1945
 1950
 1955
 1960
 1965
 1970
 1975
 1980
 1985
 1990
 1995
 2000
 2005
 2010
 2015
 2020
 2025
 2030
 2035
 2040
 2045
 2050
 2055
 2060
 2065
 2070
 2075
 2080
 2085
 2090
 2095
 2100
 2105
 2110
 2115
 2120
 2125
 2130
 2135
 2140
 2145
 2150
 2155
 2160
 2165
 2170
 2175
 2180
 2185
 2190
 2195
 2200
 2205
 2210
 2215
 2220
 2225
 2230
 2235
 2240
 2245
 2250
 2255
 2260
 2265
 2270
 2275
 2280
 2285
 2290
 2295
 2300
 2305
 2310
 2315
 2320
 2325
 2330
 2335
 2340
 2345
 2350
 2355
 2360
 2365
 2370
 2375
 2380
 2385
 2390
 2395
 2400
 2405
 2410
 2415
 2420
 2425
 2430
 2435
 2440
 2445
 2450
 2455
 2460
 2465
 2470
 2475
 2480
 2485
 2490
 2495
 2500
 2505
 2510
 2515
 2520
 2525
 2530
 2535
 2540
 2545
 2550
 2555
 2560
 2565
 2570
 2575
 2580
 2585
 2590
 2595
 2600
 2605
 2610
 2615
 2620
 2625
 2630
 2635
 2640
 2645
 2650
 2655
 2660
 2665
 2670
 2675
 2680
 2685
 2690
 2695
 2700
 2705
 2710
 2715
 2720
 2725
 2730
 2735
 2740
 2745
 2750
 2755
 2760
 2765
 2770
 2775
 2780
 2785
 2790
 2795
 2800
 2805
 2810
 2815
 2820
 2825
 2830
 2835
 2840
 2845
 2850
 2855
 2860
 2865
 2870
 2875
 2880
 2885
 2890
 2895
 2900
 2905
 2910
 2915
 2920
 2925
 2930
 2935
 2940
 2945
 2950
 2955
 2960
 2965
 2970
 2975
 2980
 2985
 2990
 2995
 3000
 3005
 3010
 3015
 3020
 3025
 3030
 3035
 3040
 3045
 3050
 3055
 3060
 3065
 3070
 3075
 3080
 3085
 3090
 3095
 3100
 3105
 3110
 3115
 3120
 3125
 3130
 3135
 3140
 3145
 3150
 3155
 3160
 3165
 3170
 3175
 3180
 3185
 3190
 3195
 3200
 3205
 3210
 3215
 3220
 3225
 3230
 3235
 3240
 3245
 3250
 3255
 3260
 3265
 3270
 3275
 3280
 3285
 3290
 3295
 3300
 3305
 3310
 3315
 3320
 3325
 3330
 3335
 3340
 3345
 3350
 3355
 3360
 3365
 3370
 3375
 3380
 3385
 3390
 3395
 3400
 3405
 3410
 3415
 3420
 3425
 3430
 3435
 3440
 3445
 3450
 3455
 3460
 3465
 3470
 3475
 3480
 3485
 3490
 3495
 3500
 3505
 3510
 3515
 3520
 3525
 3530
 3535
 3540
 3545
 3550
 3555
 3560
 3565
 3570
 3575
 3580
 3585
 3590
 3595
 3600
 3605
 3610
 3615
 3620
 3625
 3630
 3635
 3640
 3645
 3650
 3655
 3660
 3665
 3670
 3675
 3680
 3685
 3690
 3695
 3700
 3705
 3710
 3715
 3720
 3725
 3730
 3735
 3740
 3745
 3750
 3755
 3760
 3765
 3770
 3775
 3780
 3785
 3790
 3795
 3800
 3805
 3810
 3815
 3820
 3825
 3830
 3835
 3840
 3845
 3850
 3855
 3860
 3865
 3870
 3875
 3880
 3885
 3890
 3895
 3900
 3905
 3910
 3915
 3920
 3925
 3930
 3935
 3940
 3945
 3950
 3955
 3960
 3965
 3970
 3975
 3980
 3985
 3990
 3995
 4000
 4005
 4010
 4015
 4020
 4025
 4030
 4035
 4040
 4045
 4050
 4055
 4060
 4065
 4070
 4075
 4080
 4085
 4090
 4095
 4100
 4105
 4110
 4115
 4120
 4125
 4130
 4135
 4140
 4145
 4150
 4155
 4160
 4165
 4170
 4175
 4180
 4185
 4190
 4195
 4200
 4205
 4210
 4215
 4220
 4225
 4230
 4235
 4240
 4245
 4250
 4255
 4260
 4265
 4270
 4275
 4280
 4285
 4290
 4295
 4300
 4305
 4310
 4315
 4320
 4325
 4330
 4335
 4340
 4345
 4350
 4355
 4360
 4365
 4370
 4375
 4380
 4385
 4390
 4395
 4400
 4405
 4410
 4415
 4420
 4425
 4430
 4435
 4440
 4445
 4450
 4455
 4460
 4465
 4470
 4475
 4480
 4485
 4490
 4495
 4500
 4505
 4510
 4515
 4520
 4525
 4530
 4535
 4540
 4545
 4550
 4555
 4560
 4565
 4570
 4575
 4580
 4585
 4590
 4595
 4600
 4605
 4610
 4615
 4620
 4625
 4630
 4635
 4640
 4645
 4650
 4655
 4660
 4665
 4670
 4675
 4680
 4685
 4690
 4695
 4700
 4705
 4710
 4715
 4720
 4725
 4730
 4735
 4740
 4745
 4750
 4755
 4760
 4765
 4770
 4775
 4780
 4785
 4790
 4795
 4800
 4805
 4810
 4815
 4820
 4825
 4830
 4835
 4840
 4845
 4850
 4855
 4860
 4865
 4870
 4875
 4880
 4885
 4890
 4895
 4900
 4905
 4910
 4915
 4920
 4925
 4930
 4935
 4940
 4945
 4950
 4955
 4960
 4965
 4970
 4975
 4980
 4985
 4990
 4995
 5000
 5005
 5010
 5015
 5020
 5025
 5030
 5035
 5040
 5045
 5050
 5055
 5060
 5065
 5070
 5075
 5080
 5085
 5090
 5095
 5100
 5105
 5110
 5115
 5120
 5125
 5130
 5135
 5140
 5145
 5150
 5155
 5160
 5165
 5170
 5175
 5180
 5185
 5190
 5195
 5200
 5205
 5210
 5215
 5220
 5225
 5230
 5235
 5240
 5245
 5250
 5255
 5260
 5265
 5270
 5275
 5280
 5285
 5290
 5295
 5300
 5305
 5310
 5315
 5320
 5325
 5330
 5335
 5340
 5345
 5350
 5355
 5360
 5365
 5370
 5375
 5380
 5385
 5390
 5395
 5400
 5405
 5410
 5415
 5420
 5425
 5430
 5435
 5440
 5445
 5450
 5455
 5460
 5465
 5470
 5475
 5480
 5485
 5490
 5495
 5500
 5505
 5510
 5515
 5520
 5525
 5530
 5535
 5540
 5545
 5550
 5555
 5560
 5565
 5570
 5575
 5580
 5585
 5590
 5595
 5600
 5605
 5610
 5615
 5620
 5625
 5630
 5635
 5640
 5645
 5650
 5655
 5660
 5665
 5670
 5675
 5680
 5685
 5690
 5695
 5700
 5705
 5710
 5715
 5720
 5725
 5730
 5735
 5740
 5745
 5750
 5755
 5760
 5765
 5770
 5775
 5780
 5785
 5790
 5795
 5800
 5805
 5810
 5815
 5820
 5825
 5830
 5835
 5840
 5845
 5850
 5855
 5860
 5865
 5870
 5875
 5880
 5885
 5890
 5895
 5900
 5905
 5910
 5915
 5920
 5925
 5930
 5935
 5940
 5945
 5950
 5955
 5960
 5965
 5970
 5975
 5980
 5985
 5990
 5995
 6000
 6005
 6010
 6015
 6020
 6025
 6030
 6035
 6040
 6045
 6050
 6055
 6060
 6065
 6070
 6075
 6080
 6085
 6090
 6095
 6100
 6105
 6110
 6115
 6120
 6125
 6130
 6135
 6140
 6145
 6150
 6155
 6160
 6165
 6170
 6175
 6180
 6185
 6190
 6195
 6200
 6205
 6210
 6215
 6220
 6225
 6230
 6235
 6240
 6245
 6250
 6255
 6260
 6265
 6270
 6275
 6280
 6285
 6290
 6295
 6300
 6305
 6310
 6315
 6320
 6325
 6330
 6335
 6340
 6345
 6350
 6355
 6360
 6365
 6370
 6375
 6380
 6385
 6390
 6395
 6400
 6405
 6410
 6415
 6420
 6425
 6430
 6435
 6440
 6445
 6450
 6455
 6460
 6465
 6470
 6475
 6480
 6485
 6490
 6495
 6500
 6505
 6510
 6515
 6520
 6525
 6530
 6535
 6540
 6545
 6550
 6555
 6560
 6565
 6570
 6575
 6580
 6585
 6590
 6595
 6600
 6605
 6610
 6615
 6620
 6625
 6630
 6635
 6640
 6645
 6650
 6655
 6660
 6665
 6670
 6675
 6680
 6685
 6690
 6695
 6700
 6705
 6710
 6715
 6720
 6725
 6730
 6735
 6740
 6745
 6750
 6755
 6760
 6765
 6770
 6775
 6780
 6785
 6790

mens as herein shown and disclosed in detail is fully capable of obtaining the objects and providing the advantages herein before stated, it is to be understood that it is merely illustrative of the presently preferred embodiments of the invention and that no limitations are intended to the details of the construction or design herein shown other than as defined in the appended claims.

Claims

1. A system for high volume processing a plurality of minute liquid specimens characterised in that it comprises:

means for separately holding said plurality of minute liquid specimens, said holding means including a plurality of separate light transparent pathways, each said pathway being in light communication with one said specimen to permit simultaneous photometric or fluorometric analysis of said plurality of liquid specimens; and

means engageable with said holding means for maintaining said plurality of liquid specimens in a temperature controlled environment to cultivate said specimens.

2. A system according to Claim 1 wherein said holding means is a microtiter tray having a base with a substantially flat underside, and having a plurality of wells formed on said base for individually receiving one said liquid specimen therein, each said well being oriented substantially perpendicular to said underside and having a bottom distanced from said underside, said tray further having a detent formed on said base around said underside.

3. A system according to Claim 1 or 2 wherein said engageable means is a support structure including a heat exchanger engageable with said detent for firmly holding said microtiter tray.

4. A system according to any one of Claims 1 to 3 wherein said temperature controlled plate is a heat sink, said support structure includes a heating element, and said system further comprises means for coordinating the operation of said heating element for heating said liquid specimens, with the operation of said heat sink to remove heat from said liquid specimens, for cyclically changing the temperature of said liquid specimen in each said well of said microtiter tray in accordance with a predetermined regimen.

5. A system according to Claim 3 wherein said heat exchanger is a heat source for conductively heating said liquid specimens held in said wells of said

microtiter tray.

6. A system according to Claim 4 or 5 wherein said heating element is a source of microwave radiation.

7. A system according to Claim 4 wherein said heating element comprises a plurality of heating probes insertable into selected said well to heat said liquid specimens in other said wells.

8. A system according to Claim 7 wherein said support structure further comprises means for coordinating the conduction of heat energy from said heating probes to said liquid specimens with the activation of said heat sink to remove heat from said liquid specimens for cyclically changing the temperature of said liquid specimen in each said well of said microtiter tray in accordance with a predetermined regimen.

9. A multi-well microtiter tray for use in a system according to any one of Claims 1 to 8 characterised in that it comprises:

a base having a substantially flat underside;

a plurality of wells formed on said base for individually receiving one said liquid specimen therein, each said well being oriented substantially perpendicular to said underside, and each said well having a bottom distanced from said underside to establish a portion of said base between said underside and said bottom of each said well; and

a detent formed on said base around said underside engageable with means on a support structure of said system.

10. A microtiter tray according to Claim 9 wherein each said well has an opening into said well and said well is substantially cylindrical in shape to define a wall, said wall of said well being tapered inwardly from said opening to said bottom of said well to facilitate receiving said liquid specimen in said well.

11. A microtiter tray according to Claim 9 or 10 wherein said bottom of each said well has a surface with sufficient optical quality to permit photometric or fluorometric measurement of characteristics of said liquid specimen in said well using light passing through said portion of said base.

12. A microtiter tray according to any one of Claims 9 to 11 wherein each said well is substantially cylindrical in shape and wherein said bottom of each said well is substantially flat.

13. A microtiter tray according to any one of Claims 9 to 11 wherein said bottom of each said well is rounded to establish a substantially hemispherical shape for said surface.
14. A microtiter tray according to any one of Claims 9 to 11 wherein said bottom of each said well is cone shaped.
15. A microtiter tray according to any one of Claims 9 to 14 wherein said base is made of a rigid clear plastic.
16. A microtiter tray according to any one of Claims 9 to 15 wherein each said well has a displaced volume of twenty microliters (20 μ l).
17. A microtiter tray according to any one of Claims 9 to 16 wherein said plurality of wells comprises eight hundred and sixty four (864) wells.
18. A microtiter tray according to Claim 17 wherein said wells are arranged in a thirty-six by twenty-four array (36x24).
19. A microtiter tray according to any one of Claims 9 to 18 further comprising at least two indentations on said base for relative registration of said microtiter tray.
20. A microtiter tray according to any one of Claims 9 to 19 wherein said base further comprises means for identifying said liquid specimens in said microtiter tray.
21. A system according to any one of Claims 1 to 8 including a microtiter tray according to any one of Claims 9 to 20.
22. A method for high volume processing a plurality of minute liquid specimens which is characterised in that it comprises the steps of:

Placing a plurality of discrete minute liquid specimens in a microtiter tray having a base with a substantially flat underside, said tray also having a plurality of wells formed on said base for individually receiving one said liquid specimen therein, each said well being oriented substantially perpendicular to said underside and having a bottom distanced from said underside;

Mounting said microtiter tray on a support structure having a heat exchanger engageable with said microtiter tray, said heat exchanger being operable to change the temperature of said liquid specimen in each said well of said microtiter tray in accordance with a predetermined regimen;


Establishing the temperature of said temperature controlled plate to cultivate said liquid specimens; and

Photometrically or fluorometrically measuring the characteristics of all said liquid specimens in said microtiter tray.
23. A method according to Claim 22 wherein said heat exchanger is a heat sink and said support structure further comprises a heating element and said method further comprises the steps of:

Transferring energy from said heating element to heat said liquid specimens in said wells of said microtiter tray;

Activating said plate to remove heat from said liquid specimens; and

Coordinating the radiation of energy from said heating element for heating said liquid specimens with the activation of said heat sink to remove heat from said liquid specimens for cyclically changing the temperature of said liquid specimens in each said well of said microtiter tray in accordance with a predetermined regimen.
24. A method according to Claim 23 wherein said transferring step is accomplished by heat radiation.
25. A method according to Claim 23 wherein said transferring step is accomplished by heat conduction.
26. A method according to any one of Claims 22 to 25 wherein said photometric or fluorometric measurements are accomplished by passing light through said underside of said base and simultaneously through said bottom of each said well.
27. A method according to Claim 23 wherein said predetermined regimen is DNA amplification, sequencing or library construction.

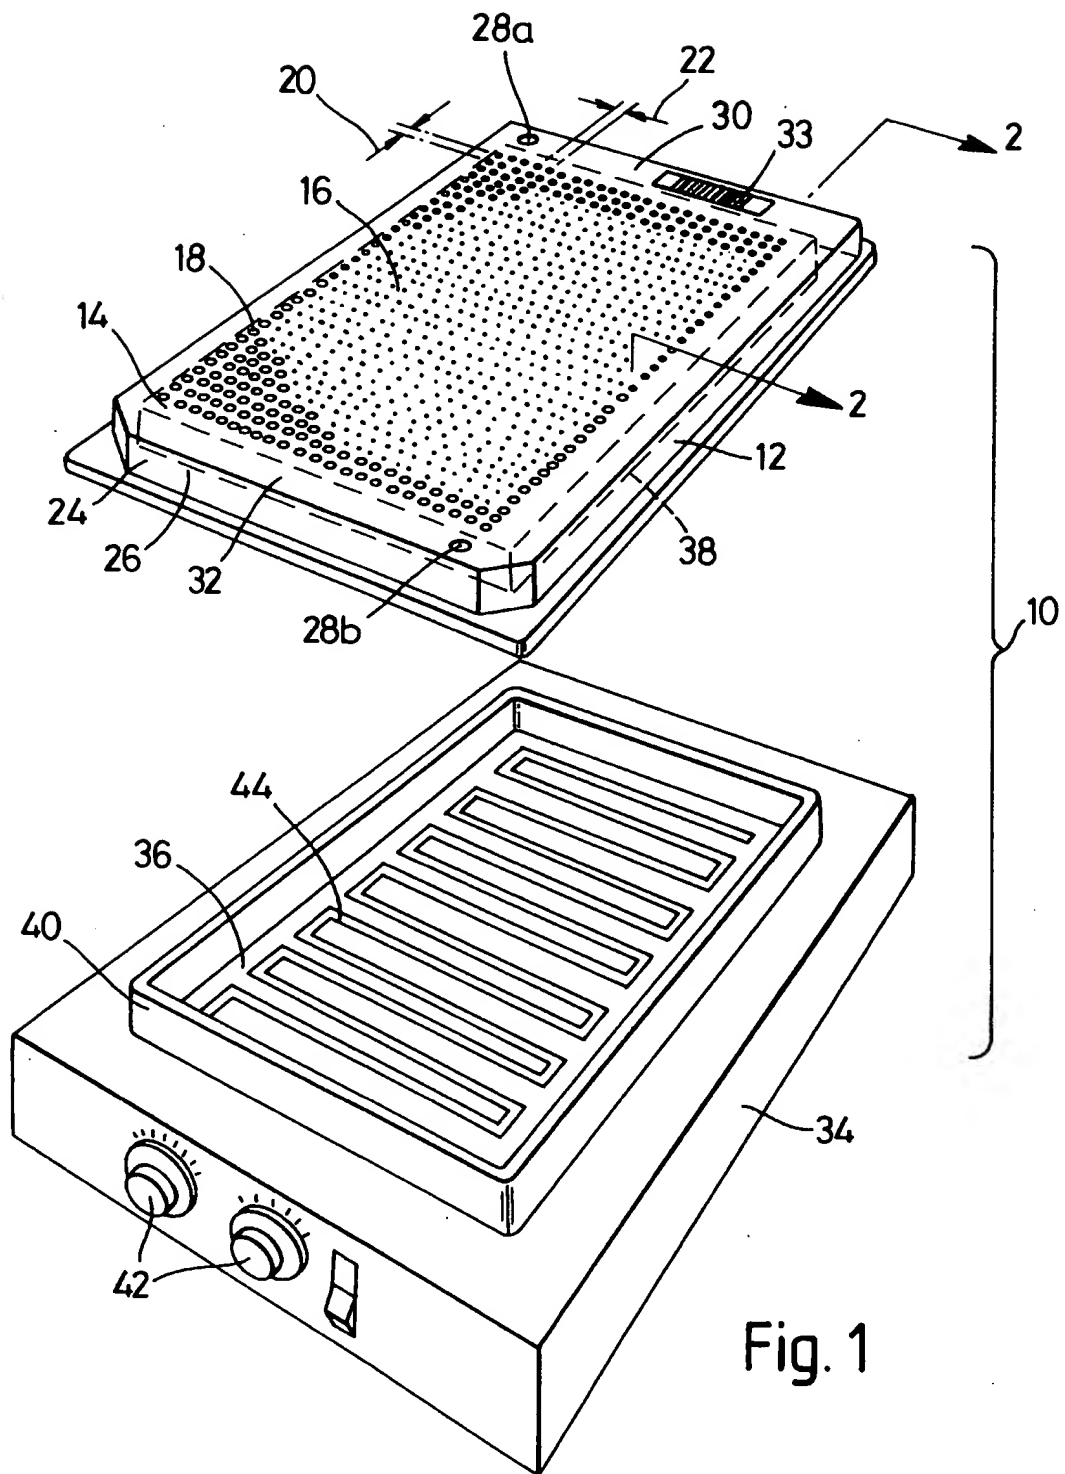

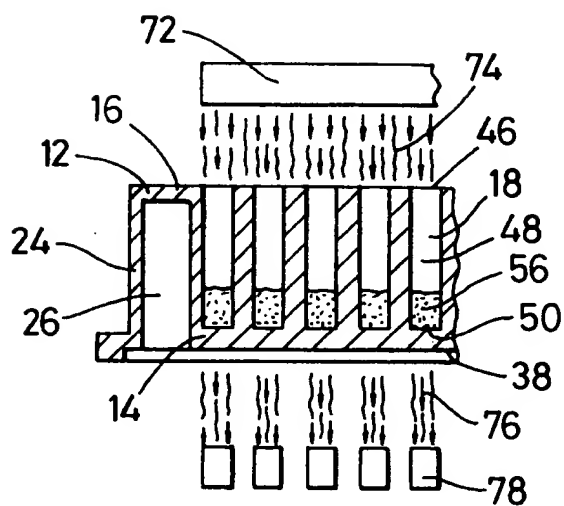


Fig. 2A

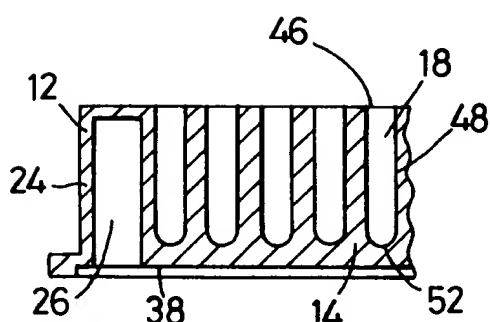


Fig. 2B

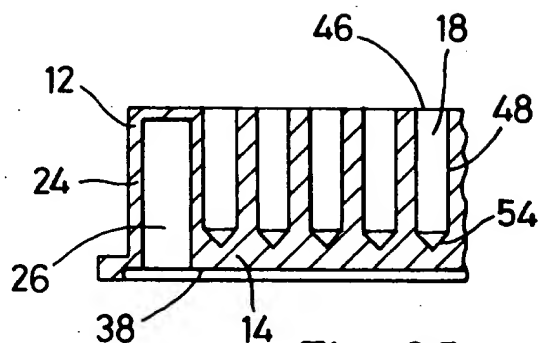


Fig. 2C







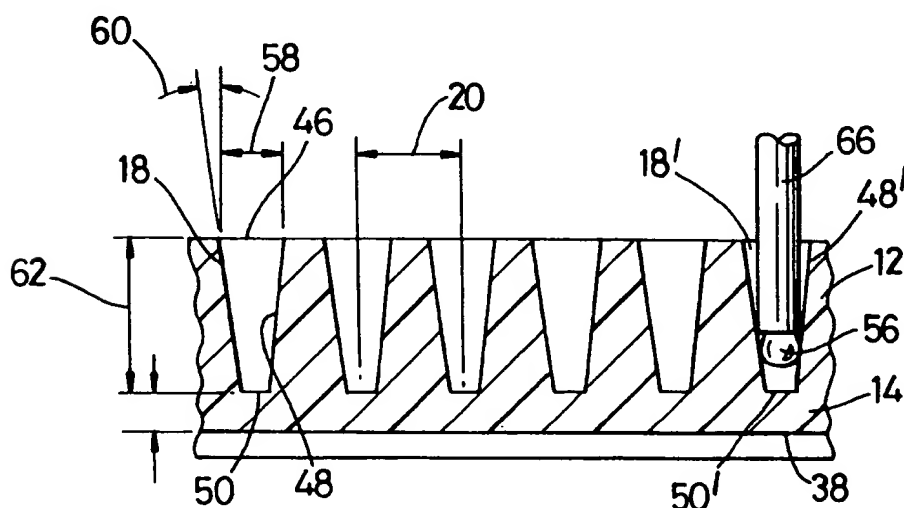


Fig. 2D

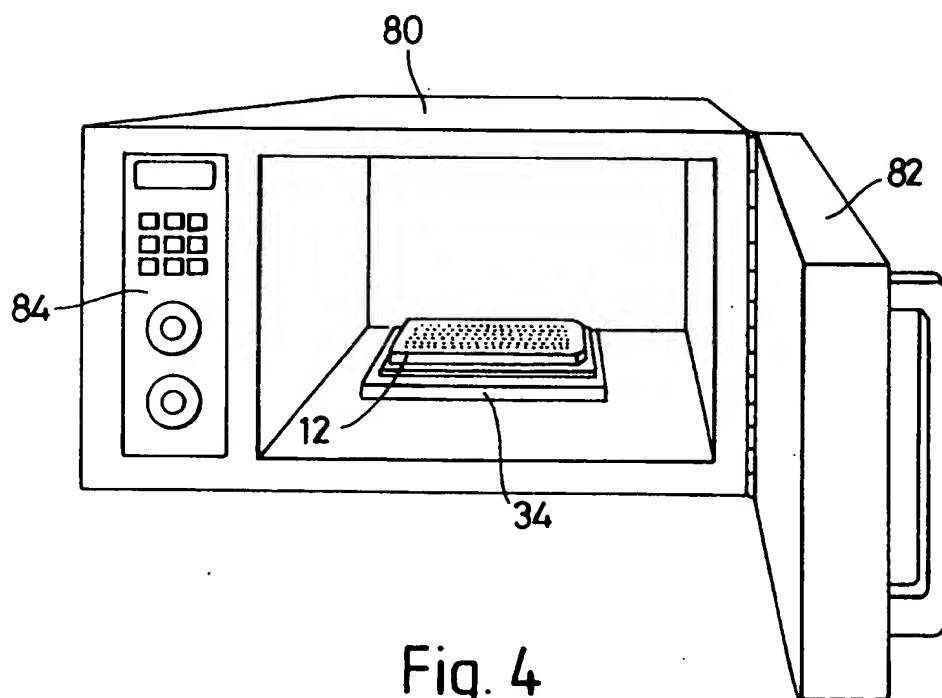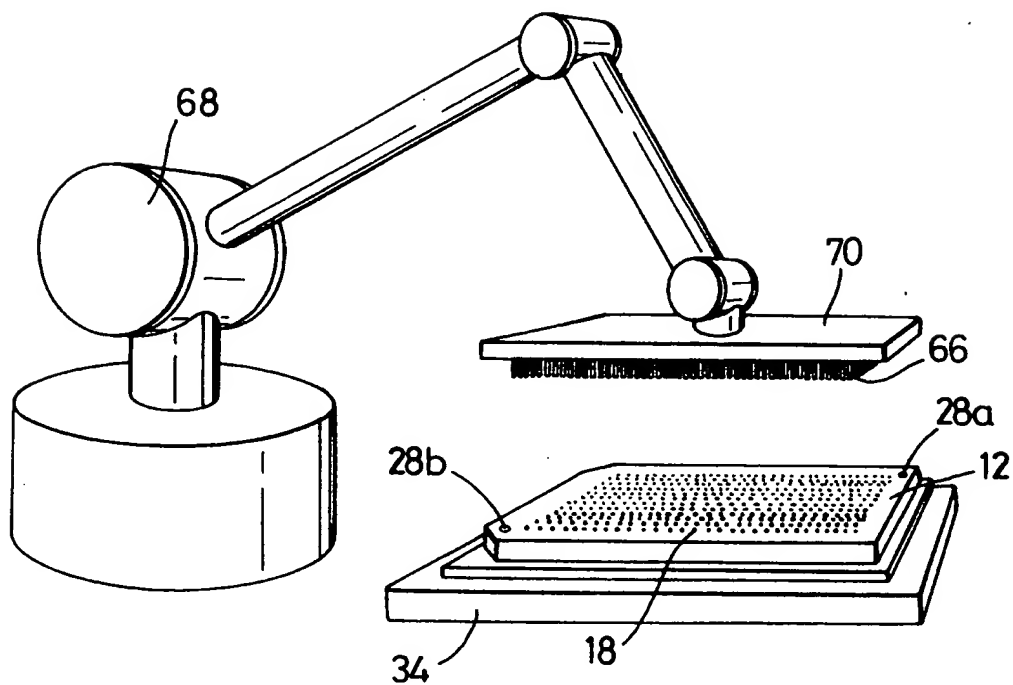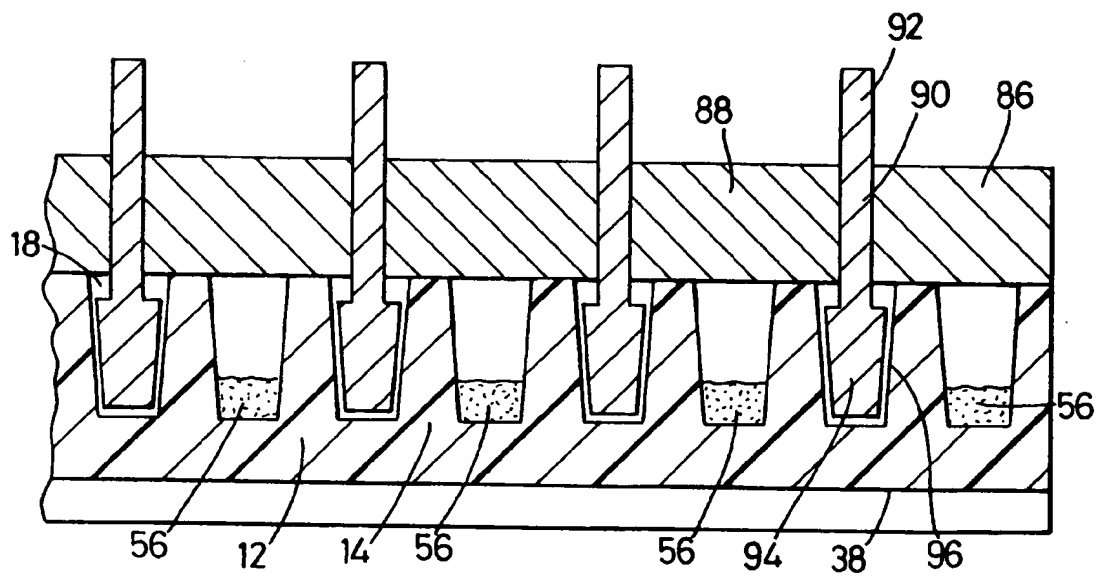

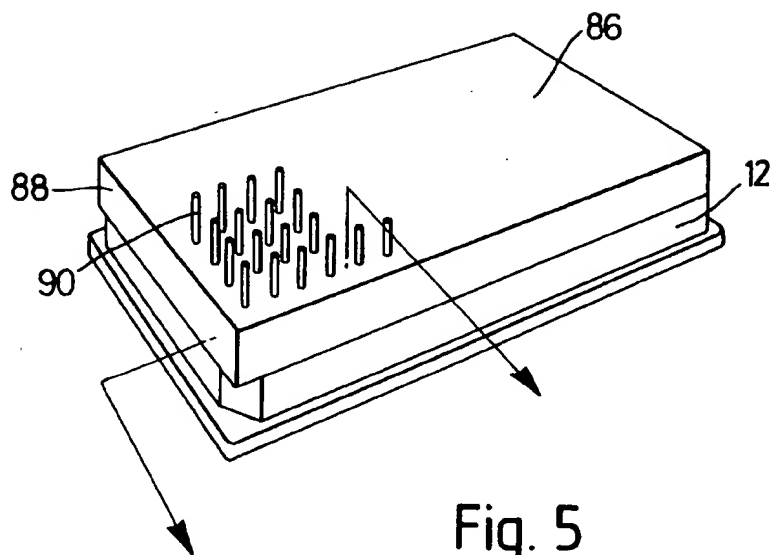

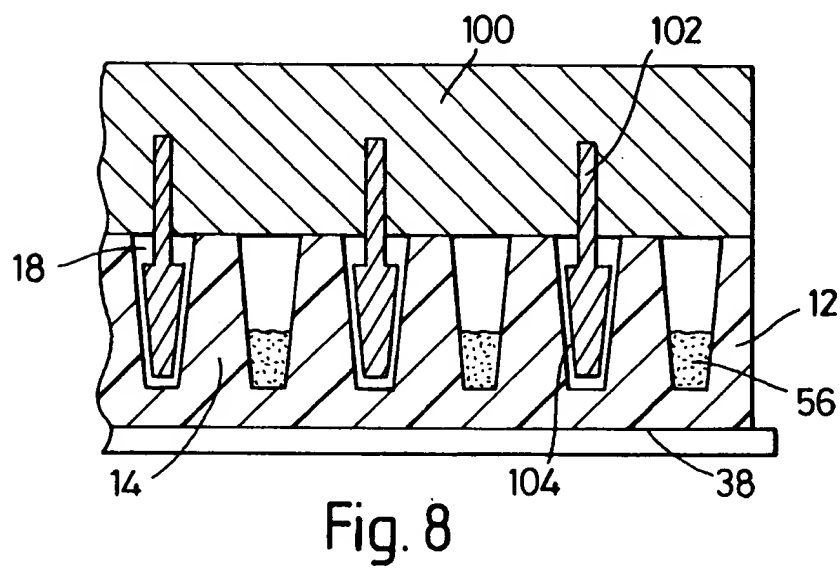

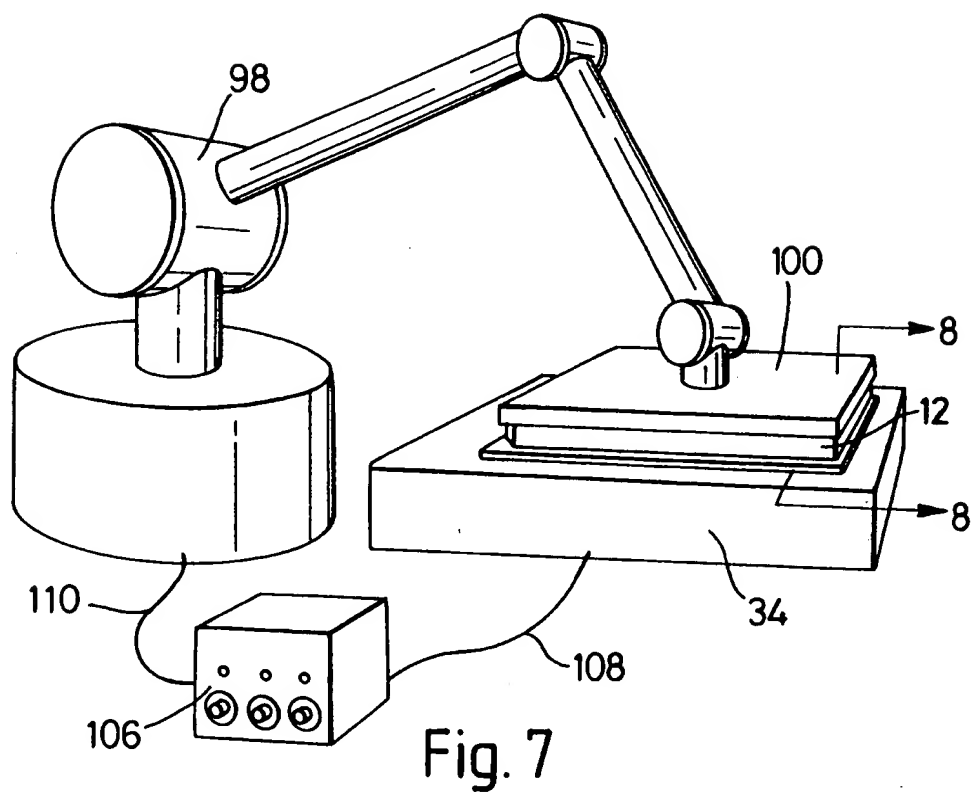

European Patent
Office

EUROPEAN SEARCH REPORT

Application Number

EP 92 30 9172

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (Int. Cl.5)
X A	EP-A-0 408 280 (TECHNE) * the whole document *	1 2-5, 9-15,21, 22,25-27	B01L3/00 B01L7/00
X A	US-A-4 599 315 (TERASAKI ET AL.) * column 3, line 62 - column 6, line 45 *	1 2,9-12, 15,16, 21,22	
X A	WO-A-8 909 437 (DEAN ET AL.) * page 5, line 1 - page 12, line 1 *	1 2,9,21, 24-27	
X A	FR-A-2 250 991 (SUOVANIEMI) * page 7, line 27 - page 10, line 17 *	1 3,9, 11-14, 19-21	
A	WO-A-8 912 502 (LEP SCIENTIFIC LTD) * page 3, line 29 - column 7, line 10 *	1-5,9,21	TECHNICAL FIELDS SEARCHED (Int. Cl.5)
A	EP-A-0 438 883 (BECKMAN INSTRUMENTS) * column 2, line 51 - column 7, line 29 *	1,3-5,9 21-23, 25,27	B01L
A	GB-A-1 528 424 (LABOR MÜSZERIPARI MÜVEK) * page 2, line 15 - line 54 *	1,2,4,7 9,10,14, 19,21,22	
The present search report has been drawn up for all claims			
Place of search THE HAGUE		Date of completion of the search 29 JANUARY 1993	Examiner BINDON C.A.
<p>CATEGORY OF CITED DOCUMENTS</p> <p>X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document</p> <p>T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document</p>			

EPO FORM 1503 01.82 (P0401)